


FIG. 1A

B

1 2 3 4

9.0 kB



6.7 kB



ICP6 (RR) PROBE

FIG. 1B

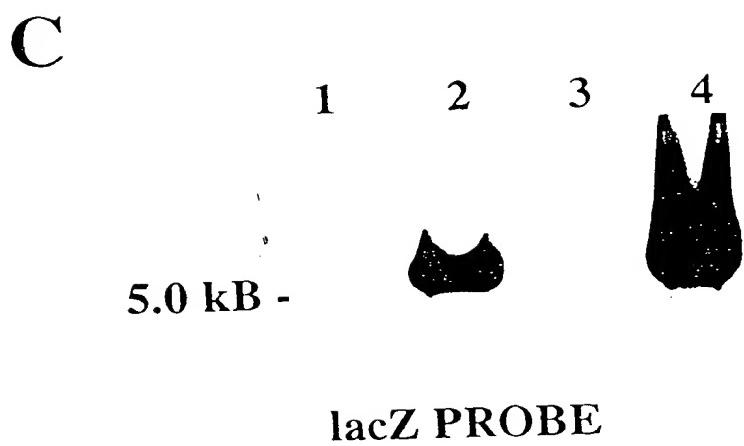


FIG. 1C

D
1 2 3 4

γ 34.5 PROBE

00011000000000000000000000000000

FIG. 1D

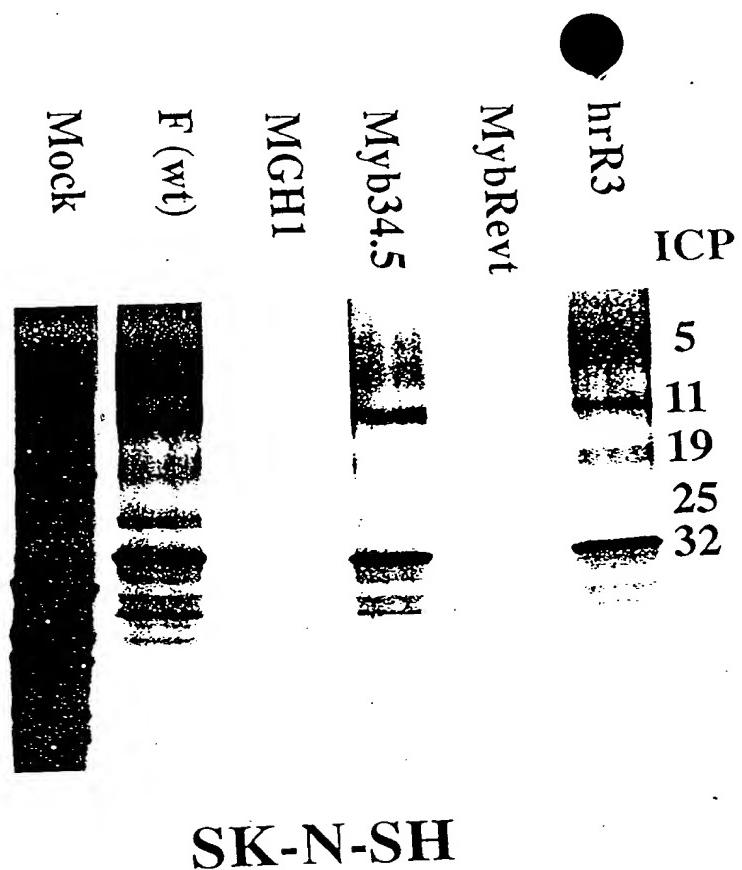


FIG. 2

□□□□□□□□□□□□□□□□□□

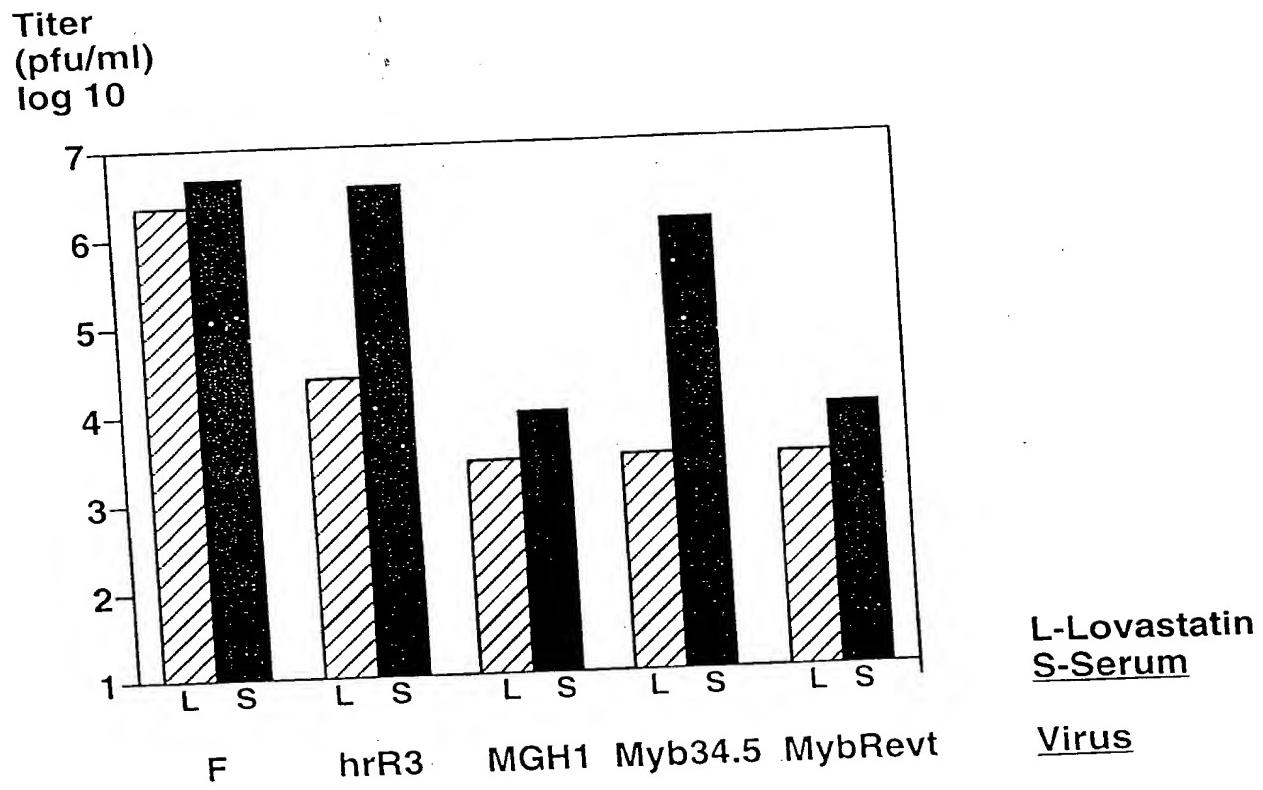


FIG. 3

A

007E30 m X 25 E960

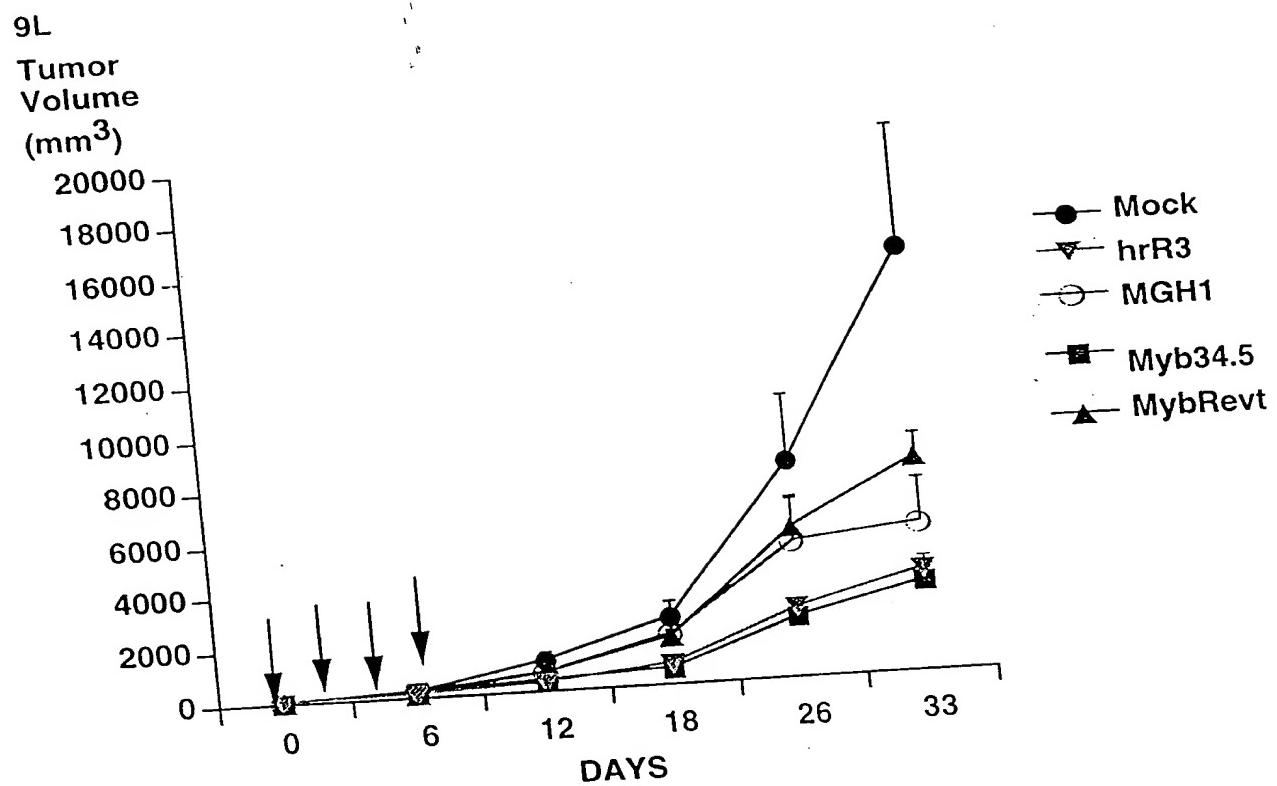


FIG. 4A

B

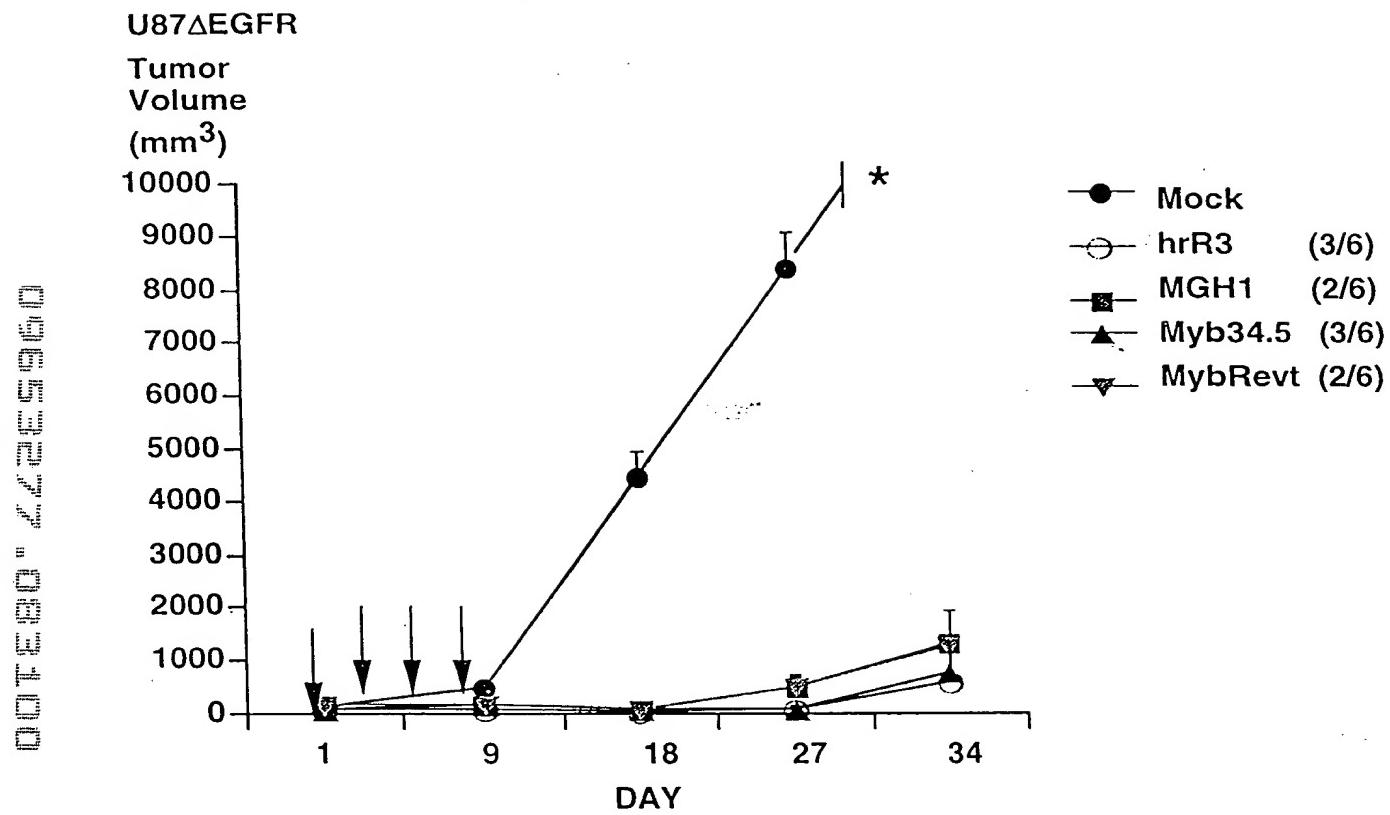


FIG. 4B

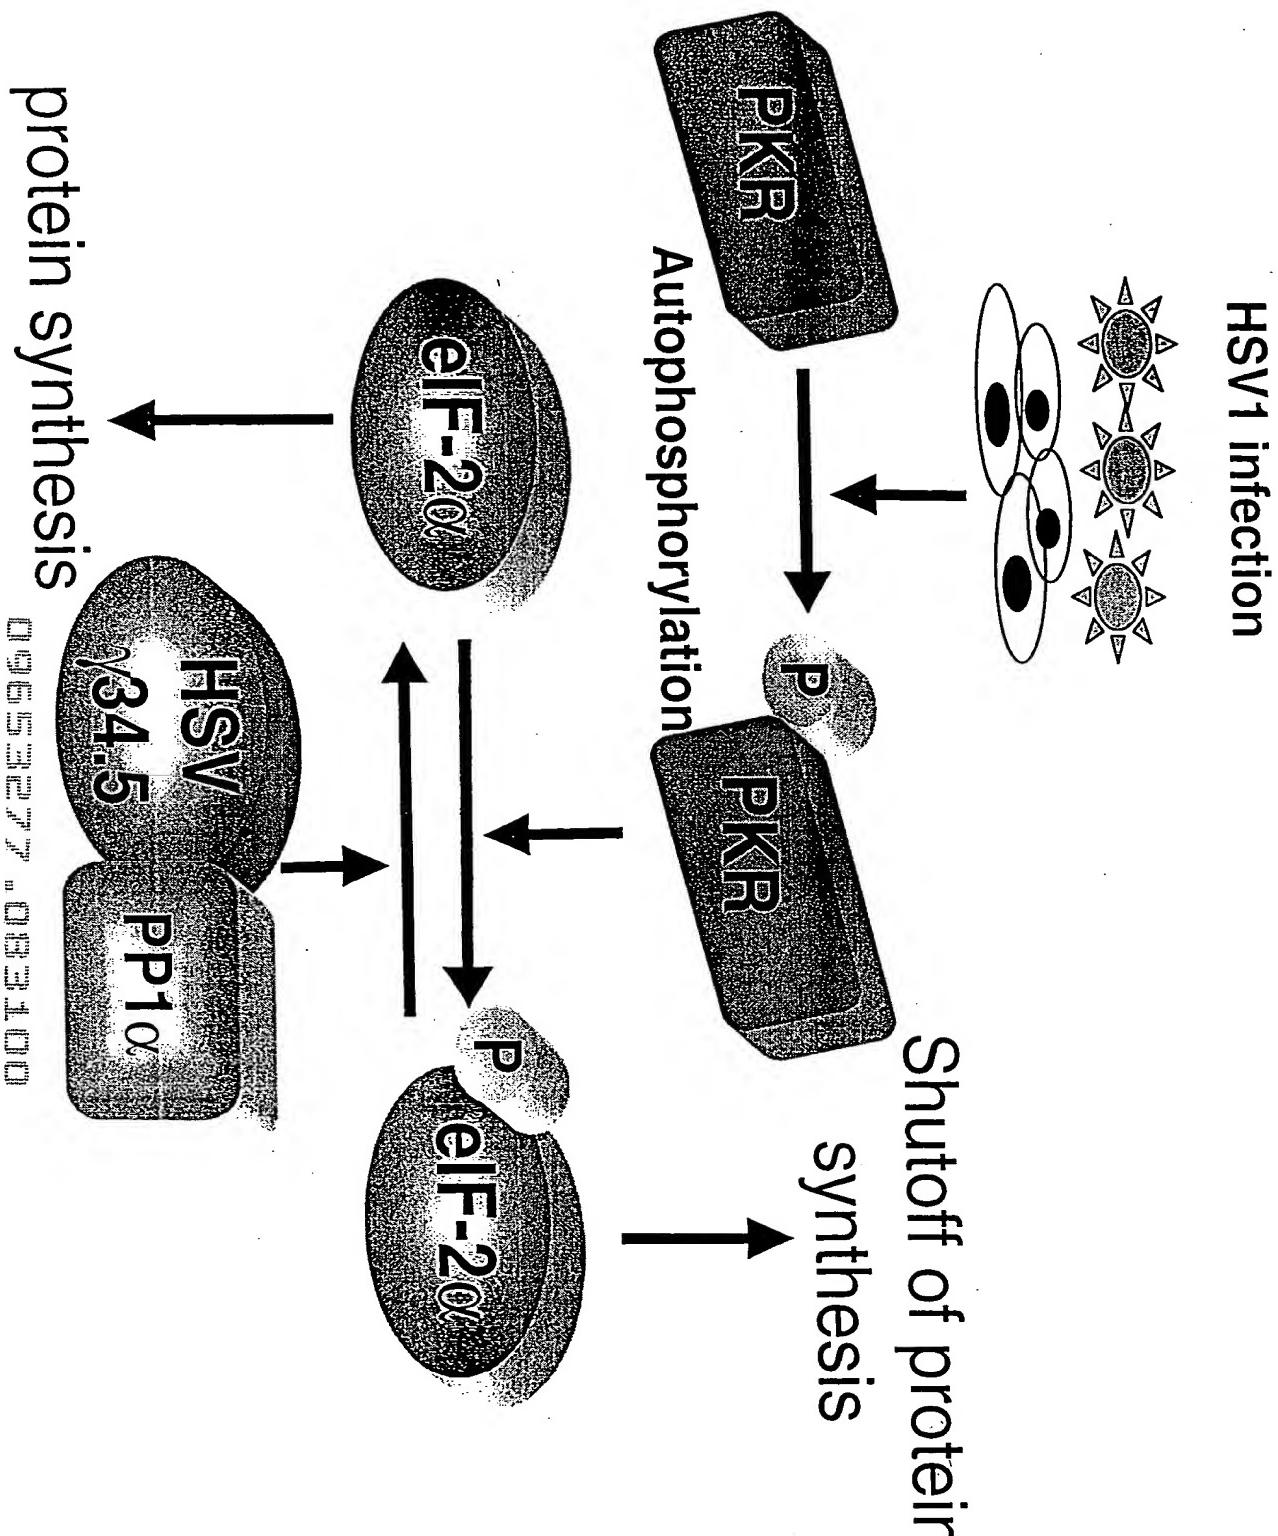


FIG. 5

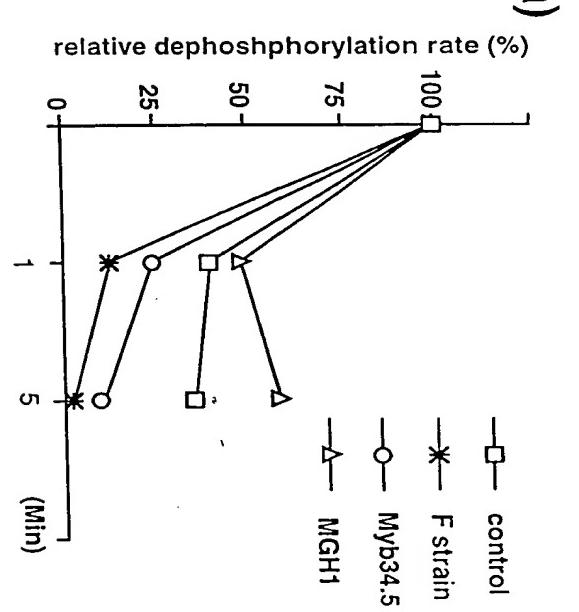
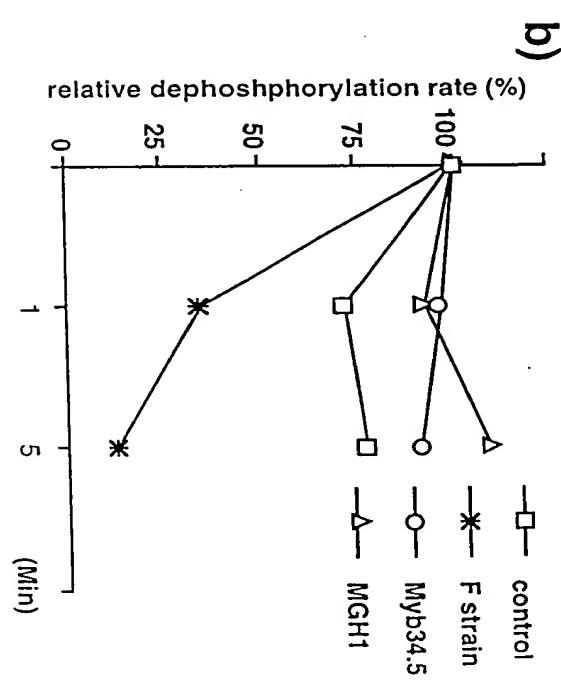
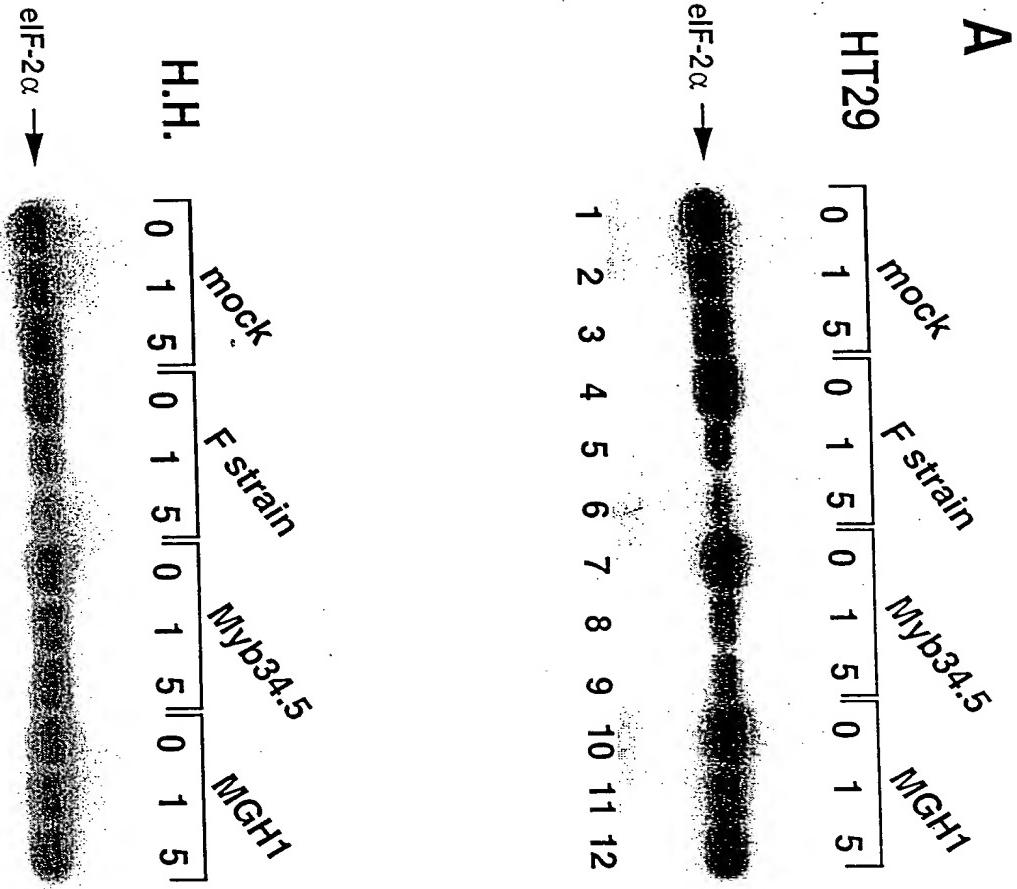


FIG. 6

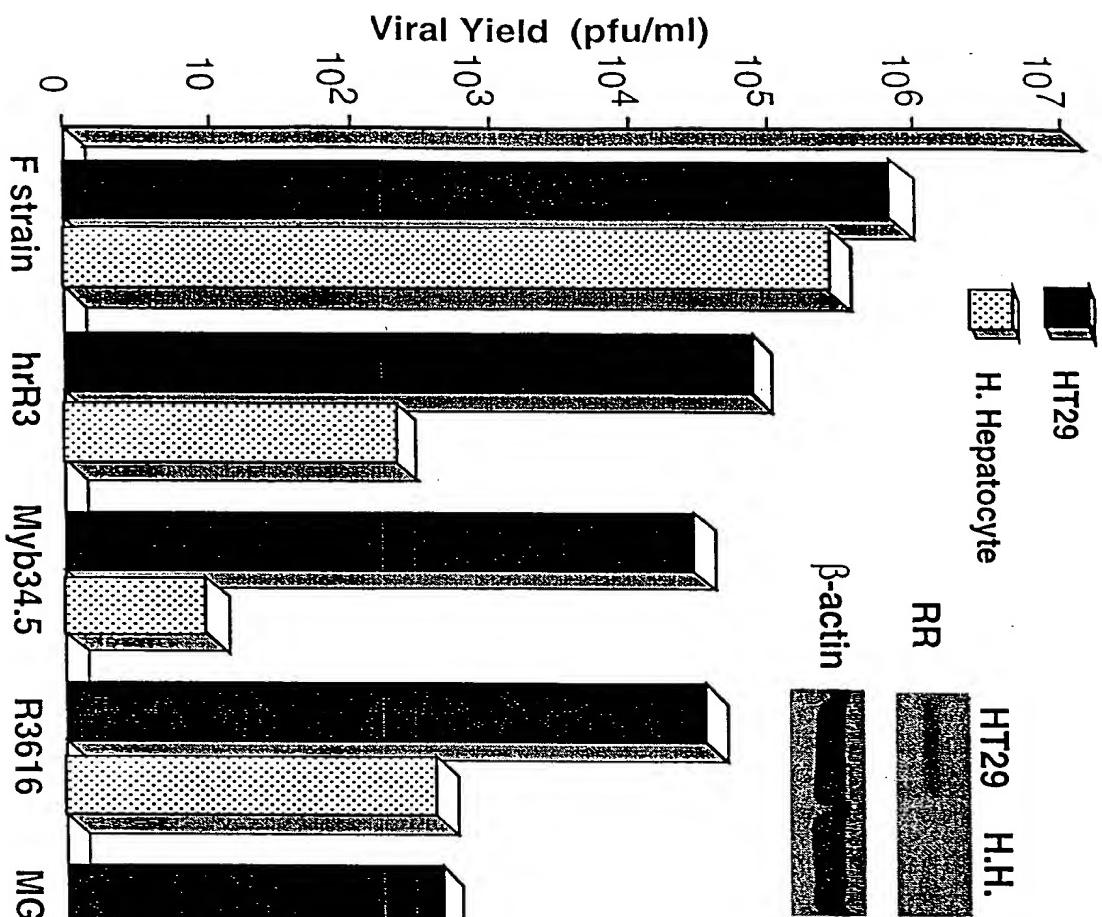
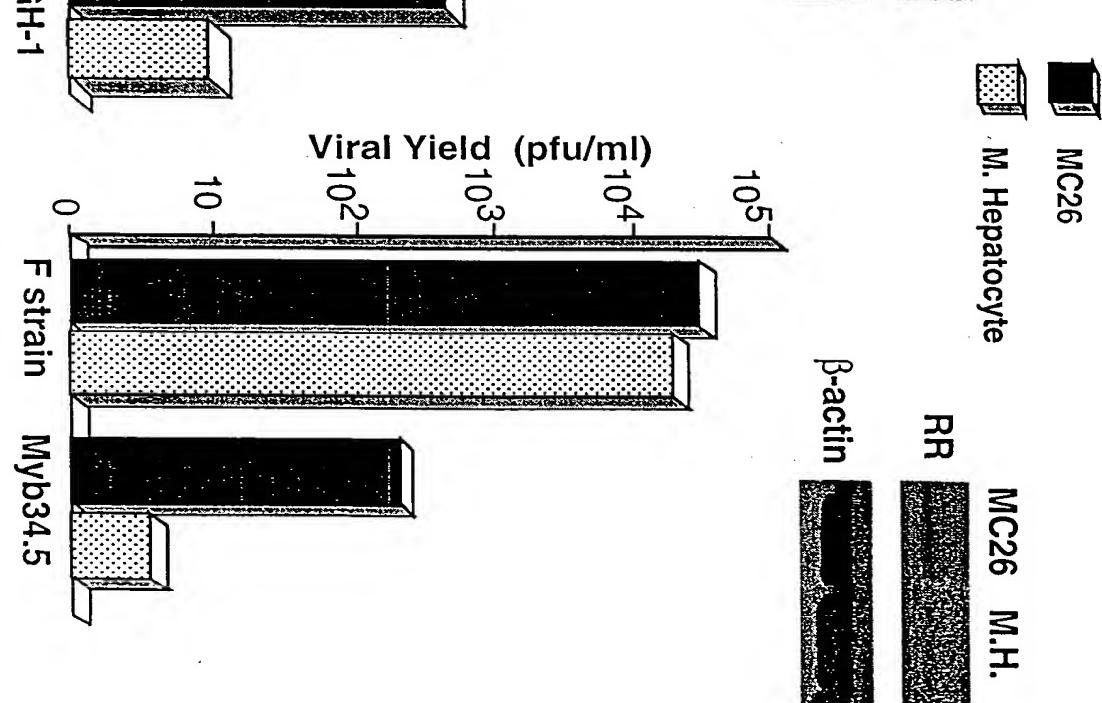
A**B****FIG. 7**

FIG. 8

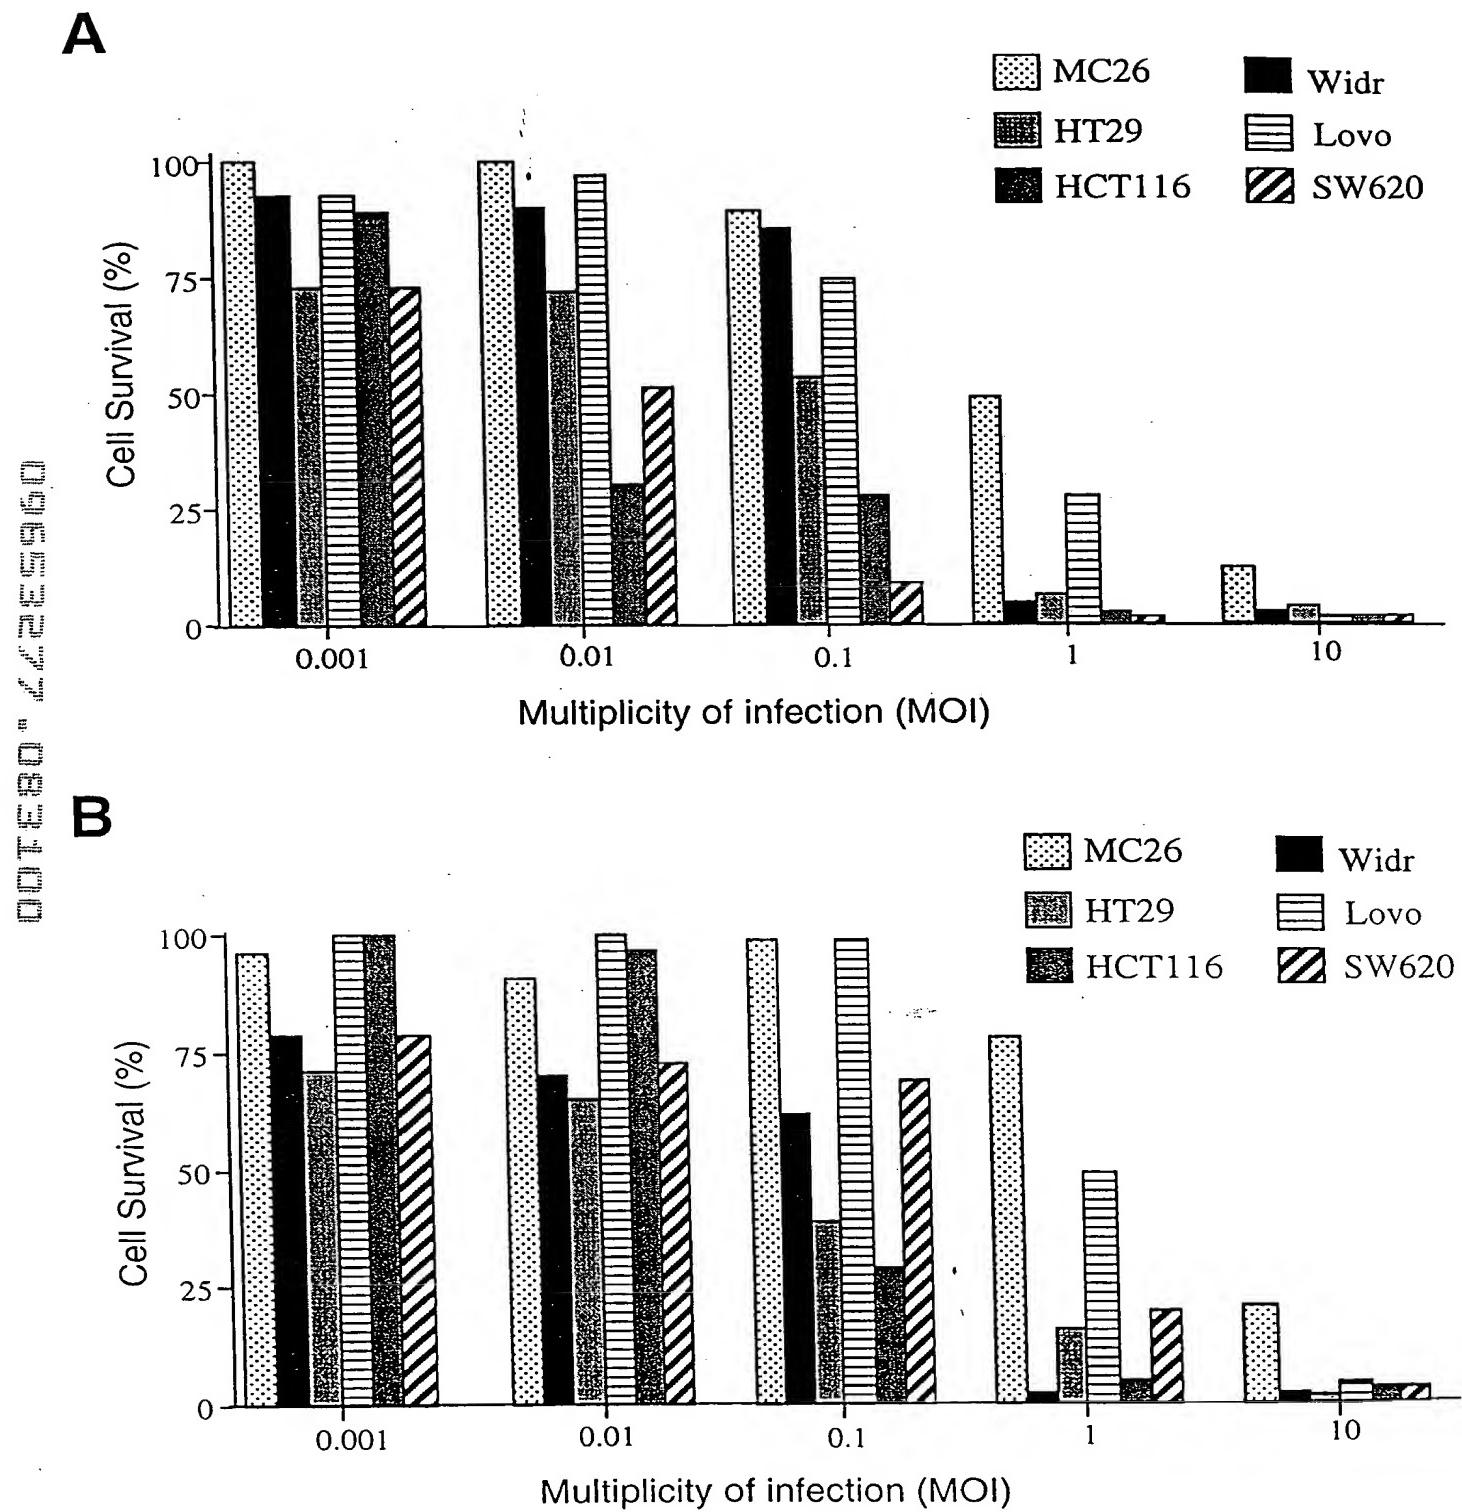




FIG. 9A

B

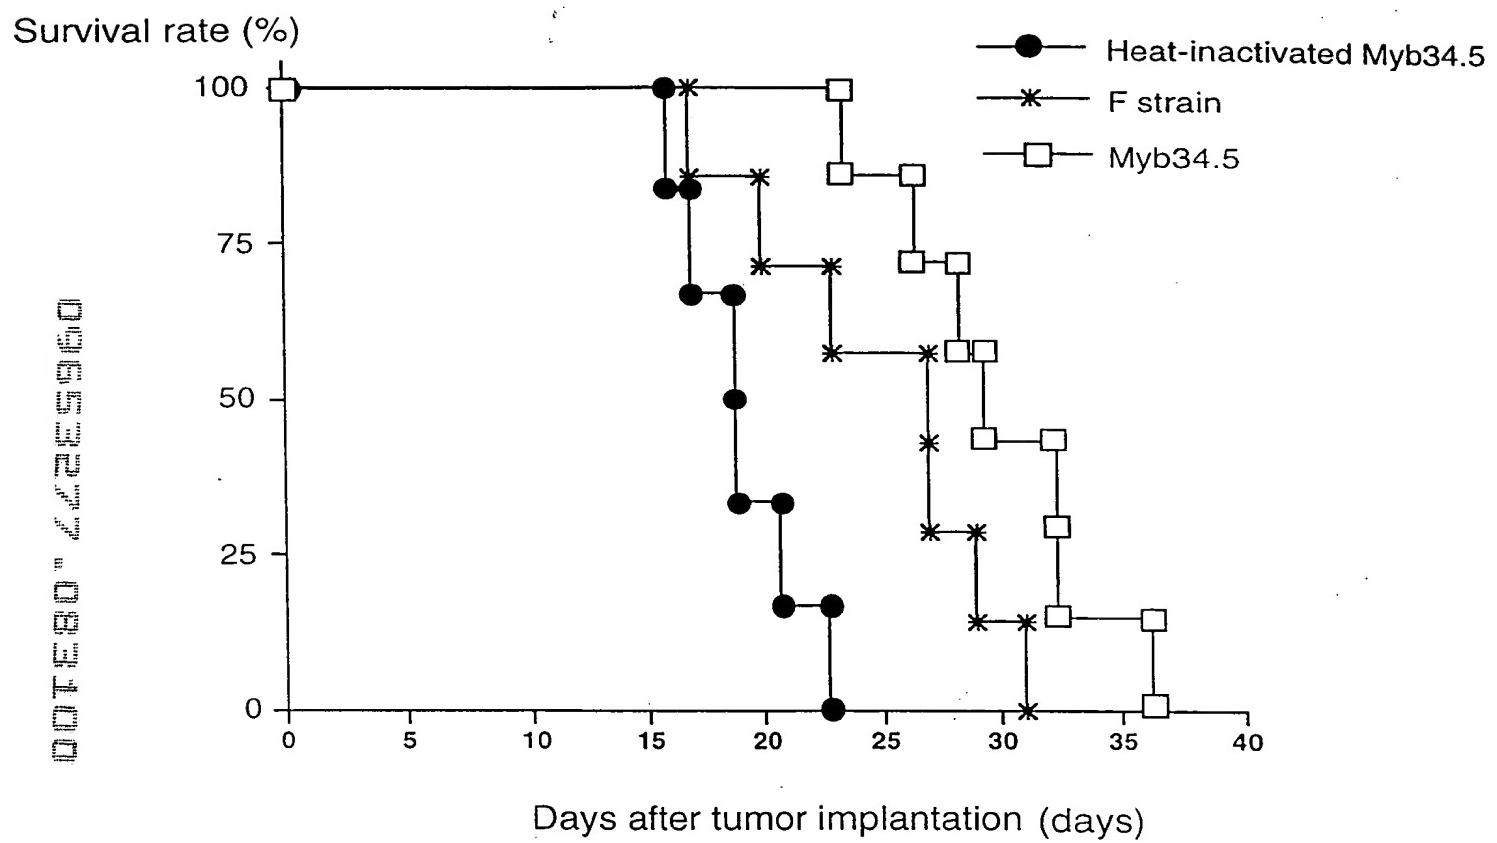


FIG. 9B


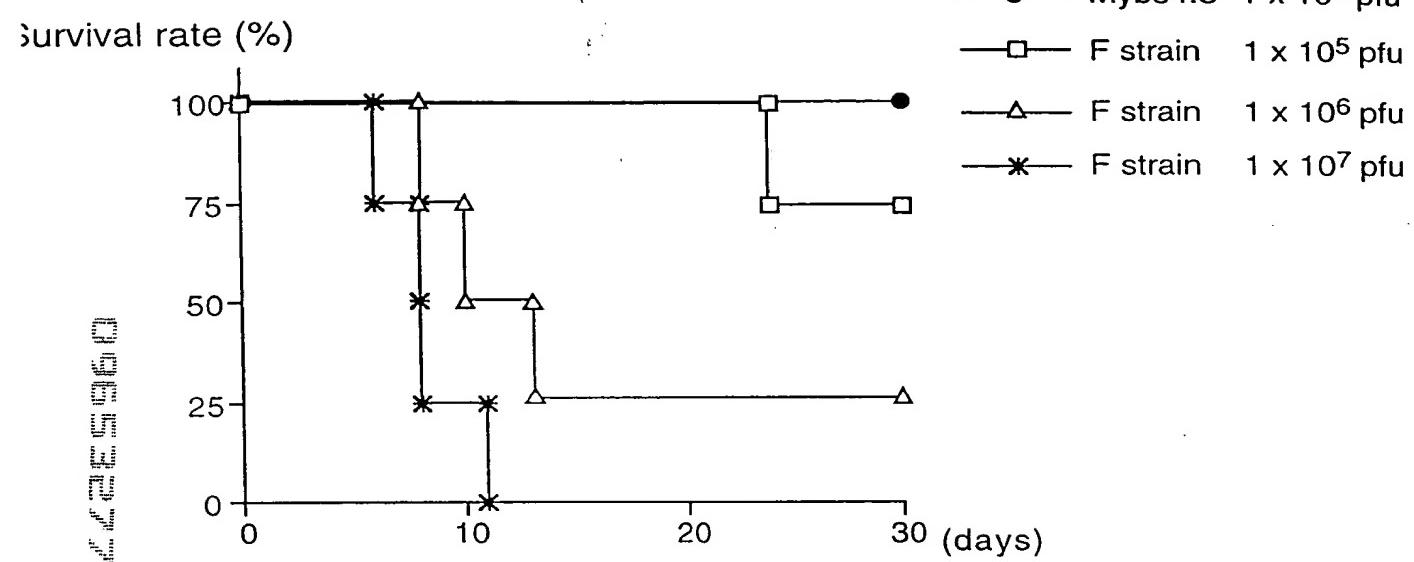


FIG. 10

A

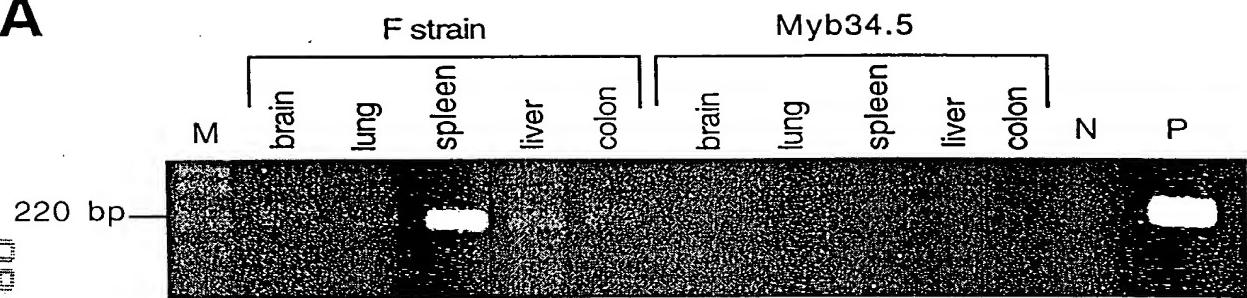

B

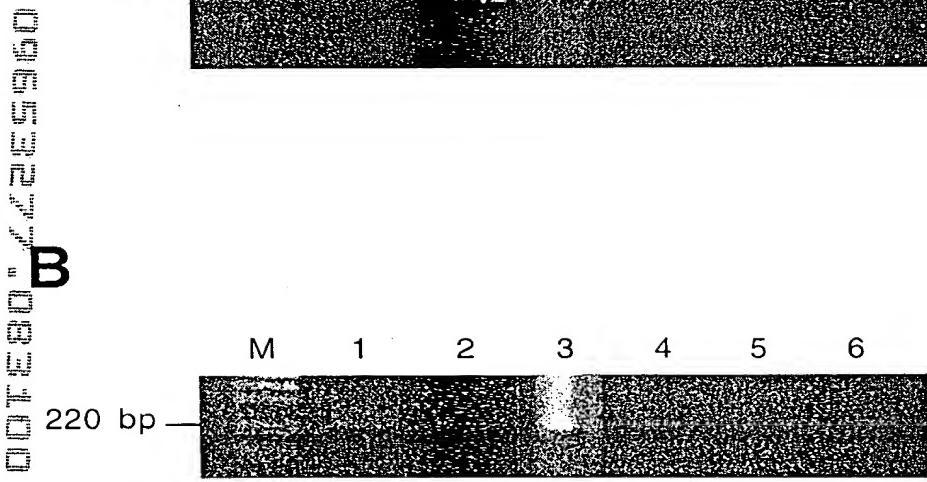


FIG. 11


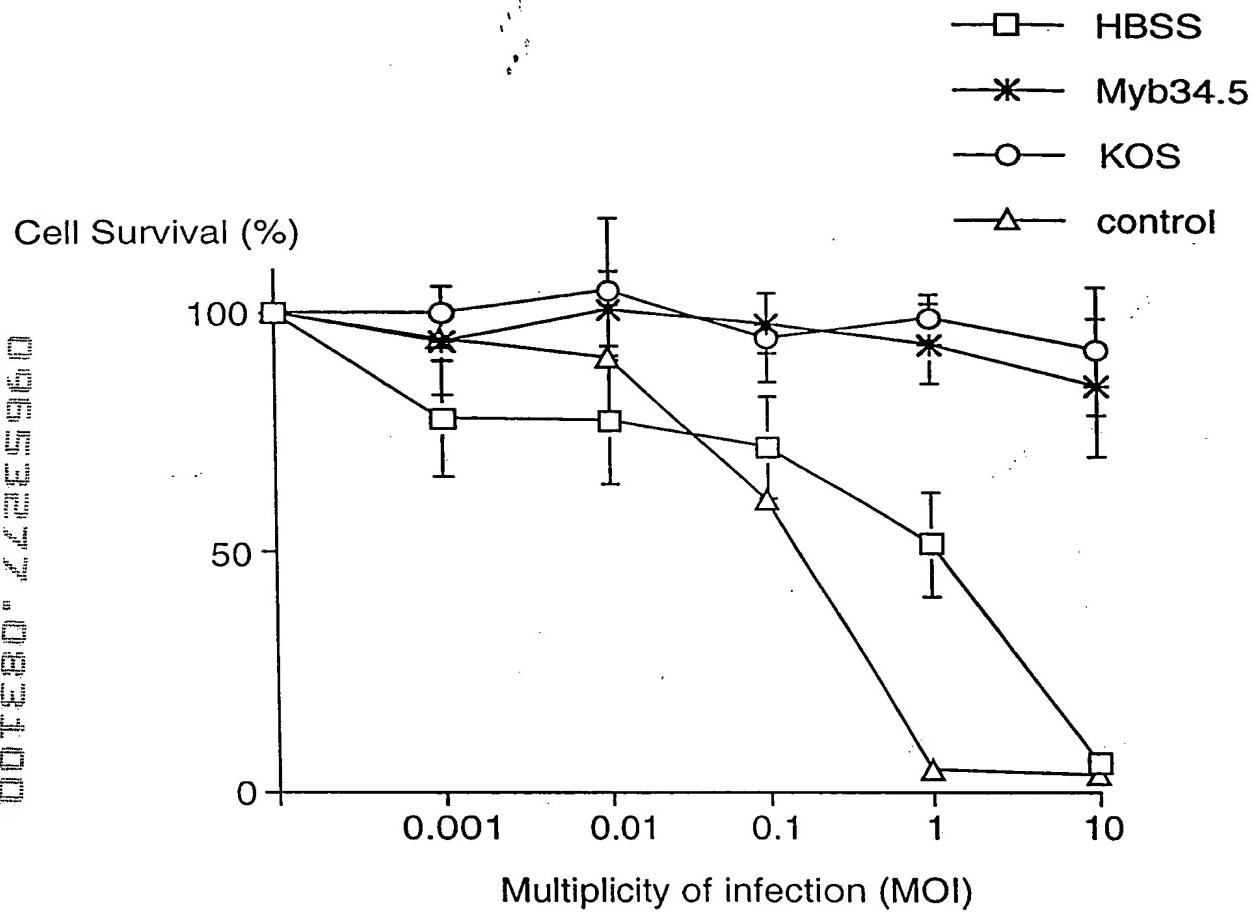


FIG. 12

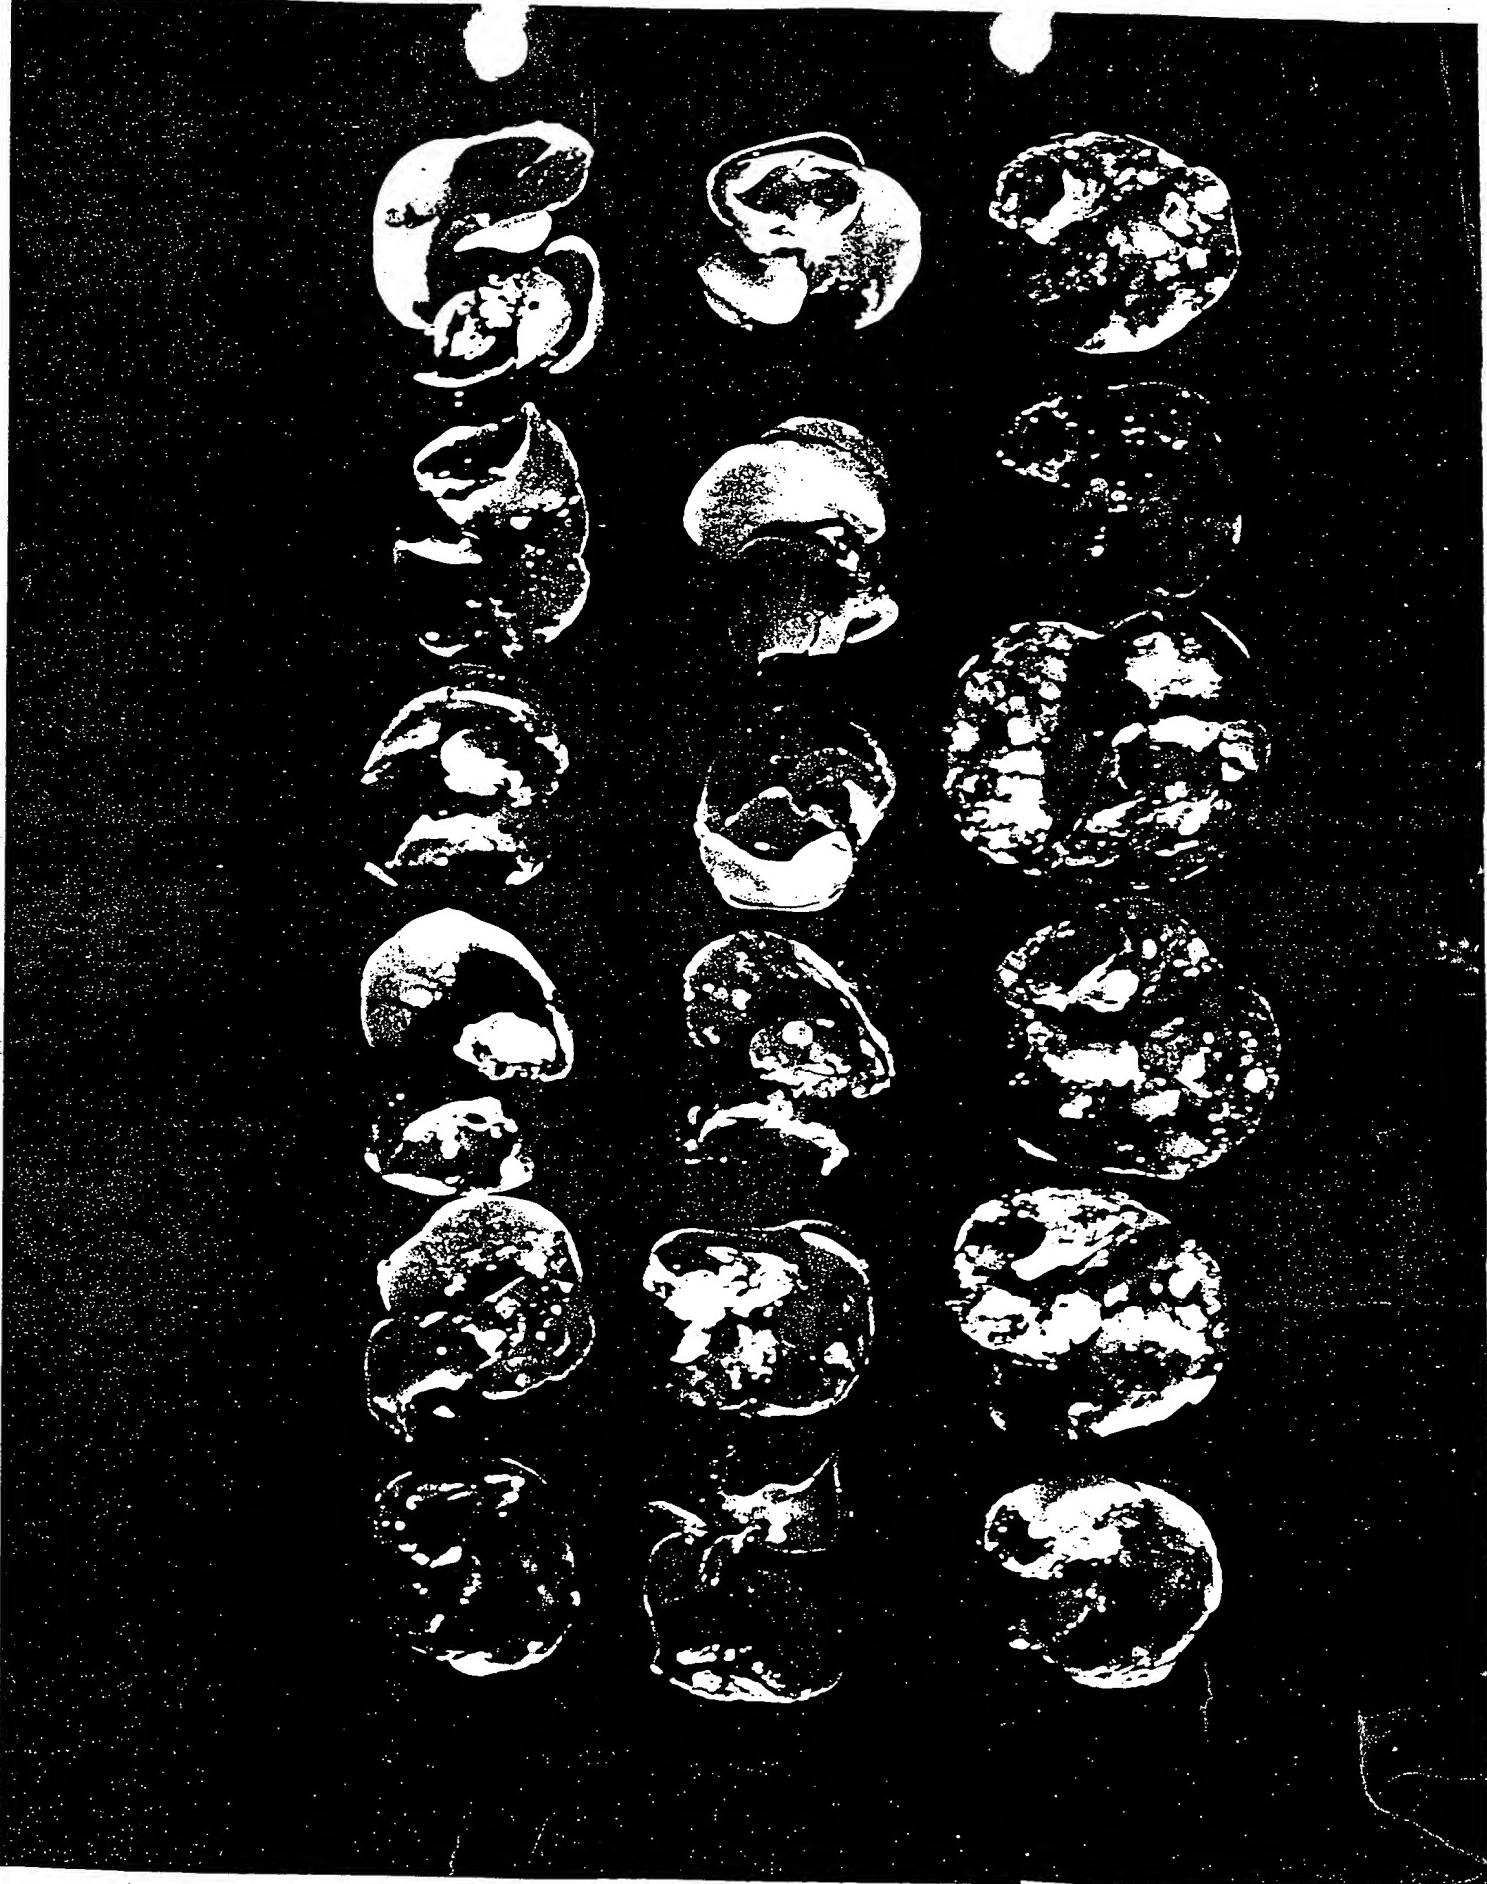

BEST AVAILABLE COPY

FIG